



CGRC ARIA II 100um 110428

Cytometer:	FACSAriaII	User:	Craig
Cytometer Name:	FACSAriaII	Institution:	ICBR Staff
Serial Number:	P46900048	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	6/1/2018 12:40:22 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


Red Laser
(633nm)

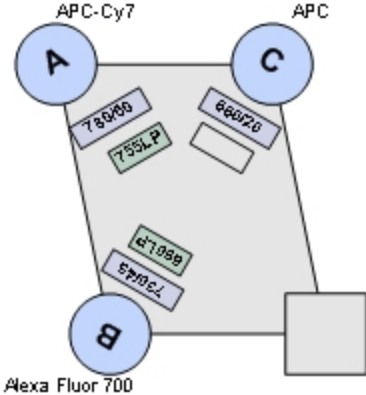


Yellow Green Laser
(561nm)

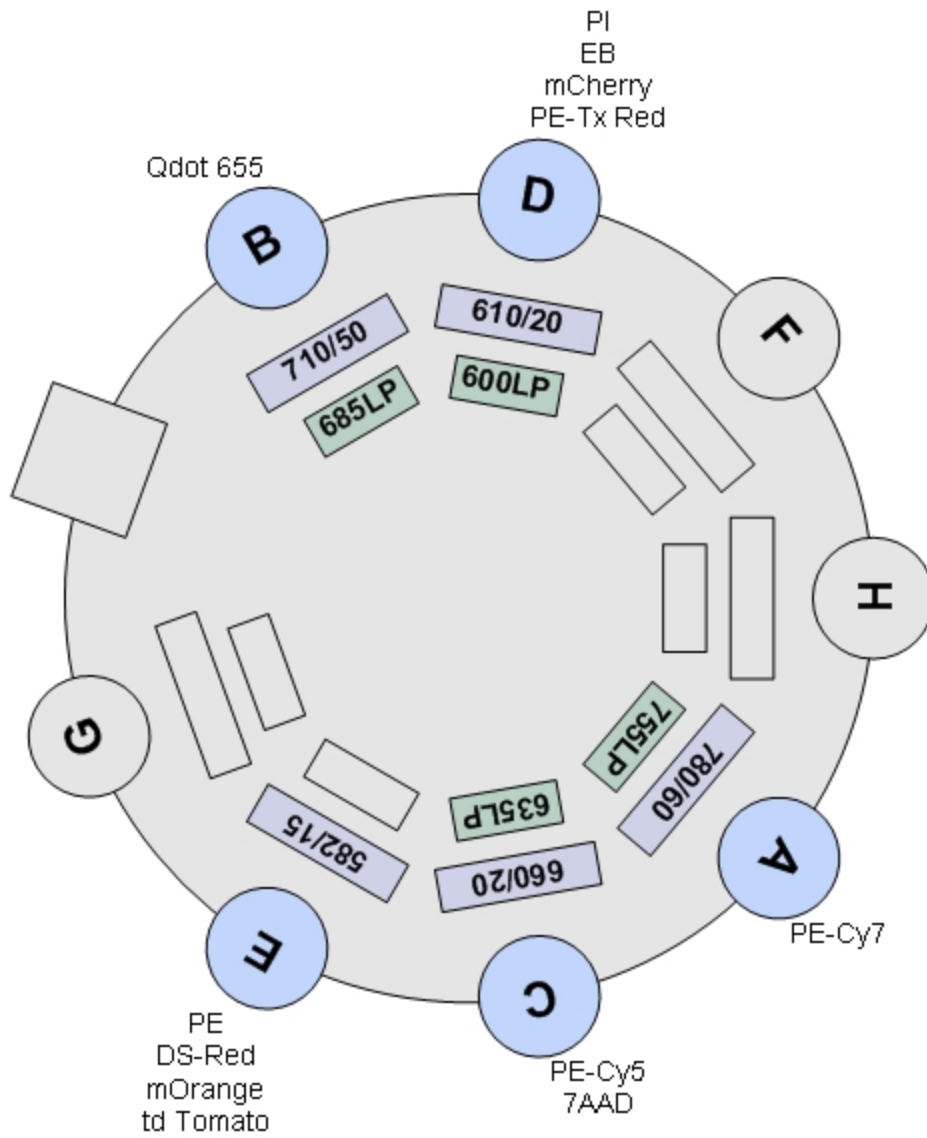


Blue Laser
(488nm)
FSC

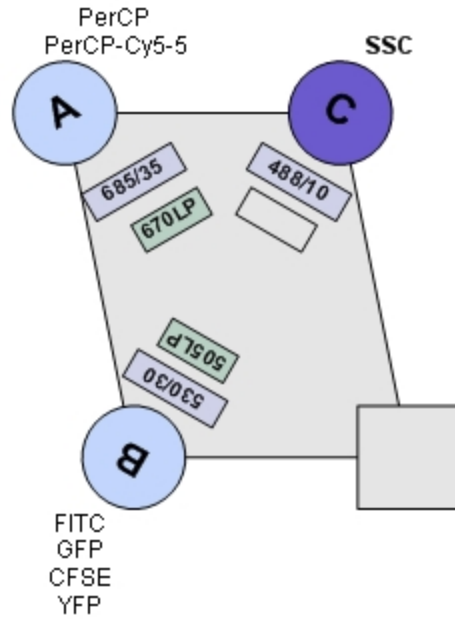

Violet Laser
(407nm)

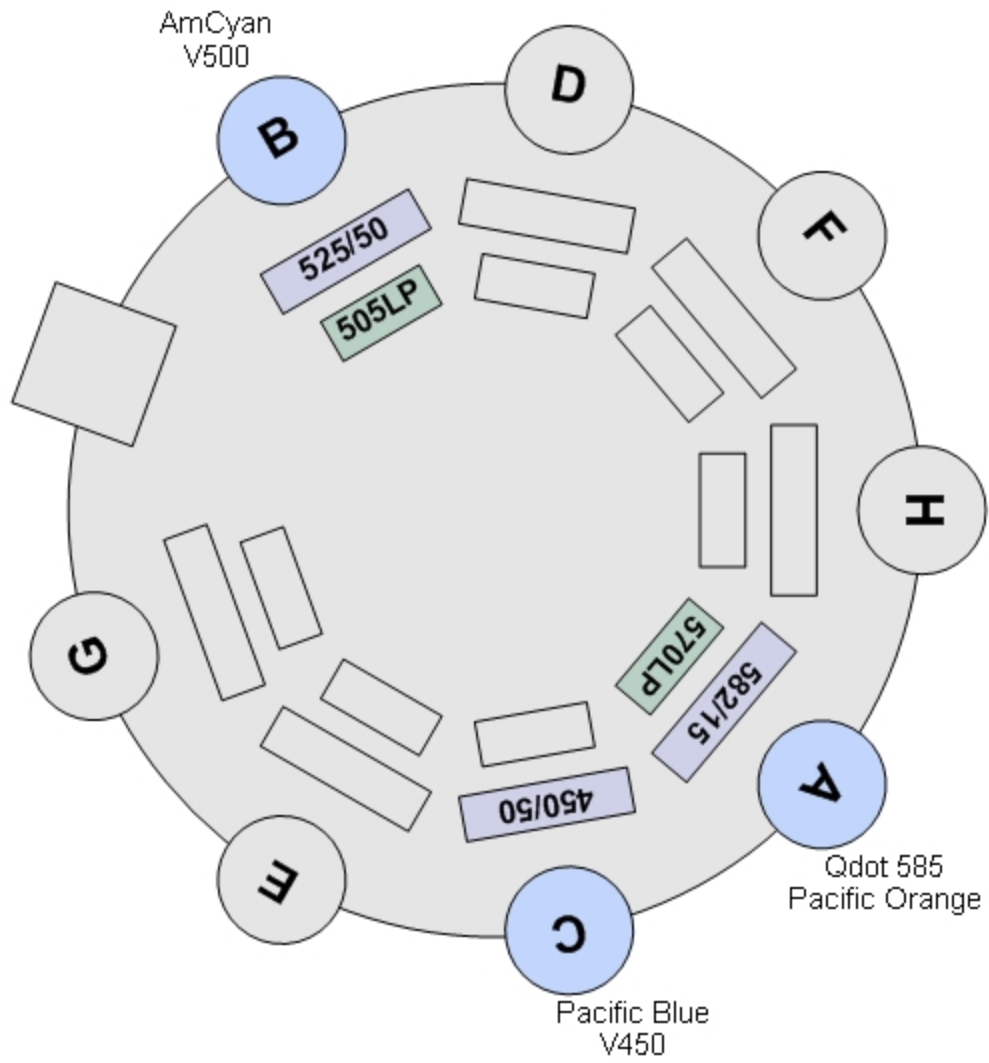

355 UV Laser
(355nm)

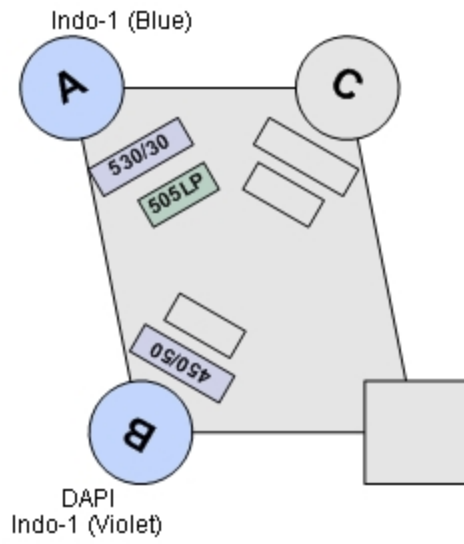

Comments: