



MBI 3-laser, 8-color (4-2-2)

Cytometer:	FACSCantoII	User:	Administrator
Cytometer Name:	FACSCantoII	Institution:	ICBR Staff
Serial Number:	V96301269	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	5/18/2018 11:40:00 AM
Window Extension:	7.00		


Blue Laser
(488nm)
FSC

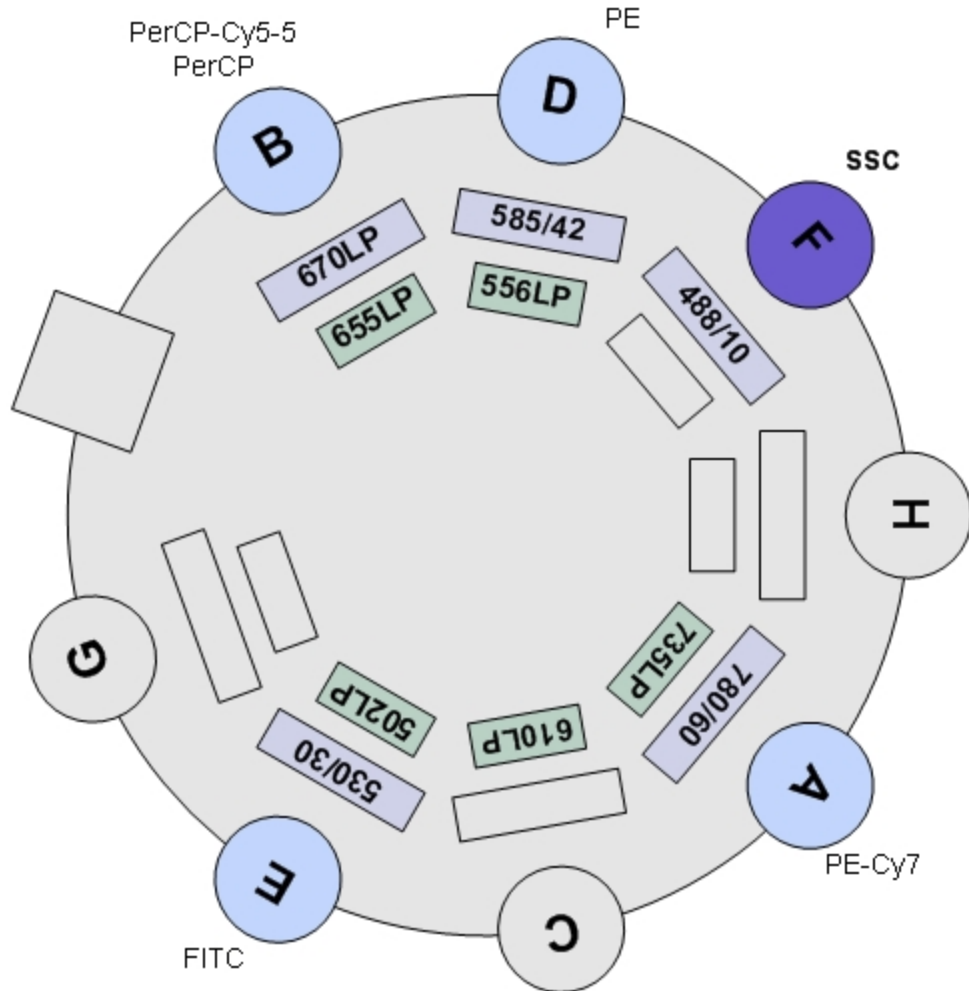

Red Laser
(633nm)

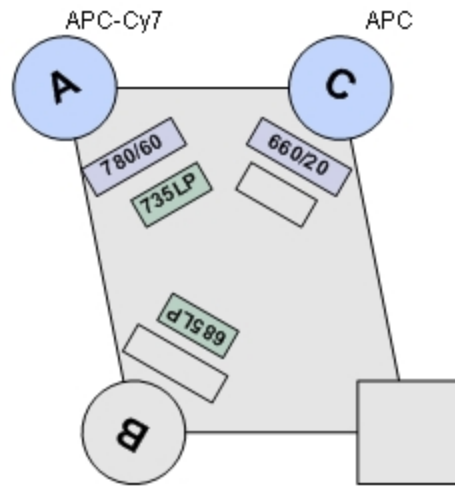

Violet Laser
(405nm)

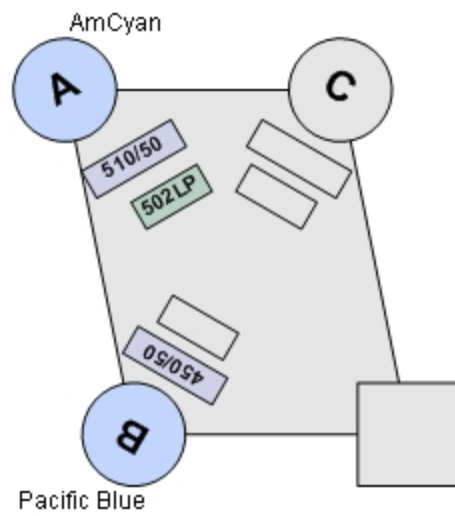

Comments: